

Calibration Certificate

This certificate guarantees that the product has been inspected and tested in accordance with the published specifications.

The instrument has been calibrated by using equipment which already calibrated to standards traceable to international standards.

Model: FT7011

Serial No.: _____

Date: _____



WATER-I.D.
WATER TESTING EQUIPMENT

WATER-I.D.

POOL-I.D. PRIMELAB EASY-DIP

Daimlerstrasse 20
D-76614 Engensteig (Baden-Württemberg)

+49 (0) 721 - 78 20 29 - 0
+49 (0) 721 - 78 20 29 - 11

www.water-id.com • info@water-id.com

WATER-I.D.
WATER TESTING EQUIPMENT

User's Guide

pH/mV/Temp
Waterproof Tester
Model: 7011



Content

Introduction	2
Features	2
Specification	3
Device Description	4
Display Description	5
Functions of Keyboard	5
Operating Procedure	6
Calibration	6 - 8
Measurement	8 - 9
Functions Mode	9
Battery Replacement	10
Electrode Replacement	10
Applications	10

Maintenance:

Battery replacement

1. Loosen the screw by screwdriver from battery compartment cap.
2. Replace the fresh AAA(UM-4) type battery, and note polarity.
3. Replace the battery compartment cap, and tighten with screw by screwdriver.

Note:

- (1) Be sure the correct position of battery by polarity
- (2) Don't lose the O-ring which has been mounted on cap.

Electrode replacement

1. Unscrew the electrode collar counterclockwise, and remove it completely.
2. Pull the electrode module out from the tester.
3. Plug an new electrode module into the tester socket carefully.
4. Replace and tighten the electrode collar to make a good seal.

Applications:

Agriculture·Anti-freeze recycling·Aquarium·Boiler·
Chemical industry·Cooling tower·Drinking water·Fish
farming·Food industry·Garden husbandry·Hydroponic·
Laboratory usage·Plating industry·Swimming pool &
Spa·Water treatment





< ORP >

1. Insert ORP electrode, and the icon **ORP** will show at LCD display automatically.
2. Rinse the electrode with clean water after calibration and wipe it dry. Dip the electrode into sample solution to be measured. Stir gently and wait until a stable reading can be obtained.

Note:

- (1) The display will appear “_ _ _ _” when it is over measuring range.
- (2) After measurement, rinse the electrode with clean water. Replace the protective cap and soaking bottle. The soaking bottle should be always kept wet by adding soaking solution.

Function mode

1. Press  button to enter hold function mode. The icon **HOLD** will appear, and the reading value can be locked shows on display. Return to measurement mode while pressing button again.
2. Press and hold  button to enter measuring maximum and minimum function mode until the display appears flash icon MAX and MIN. The value of maximum and minimum will show at display while pressing button with light. To exit this mode, press and hold  button until icon **MAX** and **MIN** disappear, and return to measurement mode.
3. Press and hold  button to change Degree °C or °F.

Introduction:

Thank you for selection model 7011 microprocessor-based waterproof pH/mV/Temp tester. It is possible to measure a wide range of pH, ORP and Temperature with a replaceable electrode. We recommend that you read and follow the manual carefully.





Features:

- ※ Large LCD displays pH and Temperature simultaneously.
- ※ Waterproof IP-57 standard and rugged design for field use conveniently. It floats on water.
- ※ Automatic Temperature Compensation (ATC) and degree °C/°F switchable.
- ※ Displays function mode automatically during insert sensor module.
- ※ Icon **PH****ORP** and unit pH, mV, °C, °F for recognition easy during select function mode.
- ※ Displays Maximum/Minimum value and data hold.
- ※ Low battery and consumption indicator. Auto shut off after 10 minutes of non use.
- ※ Easy to replace pH or ORP electrode module by user.

Specifications:

7011					
	pH	ORP	Temp.		
Range	0 - 14	± 1000	0 - 90 °C		
Accuracy	± 0.01	± 2	± 0.2 °C		
Resolution	0.01 pH	1 mV	0.1 °C		
ATC	0 - 90 °C				
Calibration	pH 4.00, 7.00, 10.01				
Power	DC1.5V × 4 battery (UM-4/AAA)				
Dimensions	Meter: 195 × 40 × 36 mm Kits: 230 × 205 × 50 mm				
Weight	Meter: 135g (with battery) Kits: 700g				

< ORP >


1. Make sure that the ORP electrode is screwed on or check that the ORP symbol is displayed on the LCD screen.
2. Immerse the electrode in the +468 mV buffer solution. Press and hold the  button to enter the calibration mode.
3. Adjust the calibration value to 468 by pressing the "Up"  or "Down"  key until 468 is displayed.
4. Press the  key again. The calibration starts now. As soon as the screen stops flashing and displays "SA" and "END", you will return to the measuring mode.
5. Rinse the electrode with clean water and then dry it.


Note:

(1) In case of a failed calibration, the symbol "SA" symbol does not appear.

Measurement

< pH >

1. Insert pH electrode, and the icon  will show at LCD display automatically
2. After calibration, rinse the electrode with clean water and wipe it dry. Dip the electrode into sample solution to be measured. Stir gently and wait until a stable reading can be obtained.

3. Rinse the electrode with clean water and wipe it dry. Dip the electrode into the buffer solution pH 4. Stir gently and wait until the display stabilized. Press and hold  button to enter calibration mode until the display appears icon **CAL**, and then flash 4.00. When the display stop flashing and indicates "%" (percentage of slope), then "SA", then "End" while calibration is ending, and return to measurement mode.
4. After slope calibration pH 4 or pH 10, the display will indicate percentage of slope (PTS) to show the status of electrode. If the PTS is below 70% or above 130%, the electrode must be replaced. A slope of 100% is ideal.


Note:

- (1) Icon "SA" will not appear if the calibration fails.
- (2) When doing a 2 or 3 point calibration, Calibrate with buffer pH 7 first, and then follow with buffer pH 4 or pH 10.

Device Description:




Display Description:

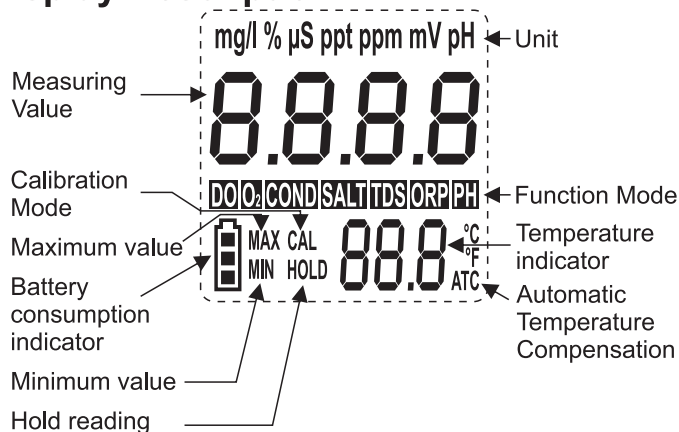


Functions of keyboard:


Power/Calibration

1. Press button to switch power On or Off. 
2. Press and hold button to enter calibration mode.

Function Mode

1. Press and hold button to change degree °C or °F. 

Hold/Max & Min

1. Press button to enter Hold mode. 
2. Press and hold button to enter Maximum/Minimum mode.
Press button with light to get Maximum and Minimum value.
3. Press and hold button again to exit this mode and return to measurement mode.


Operating procedure:

Accessories

Upon receiving the shipment, inspect the container and equipment for any signs of damage. Remove the packing list and verify that you have received all equipments:


Meter, Buffer solution pH 4 & 7, Soaking solution, Lanyard, Battery, Instruction manual, Carrying case.
Optional: ORP electrode, Buffer pH 10.01

Preparation

1. Remove the protection cap and unscrew soaking bottle from meter to rinse the electrode with clean water and wipe it dry. Don't leak soaking solution from bottle, and replace bottle when end of usage.
2. Press  button to turn the meter power on.

Calibration

< pH >

1. Make sure the sensor is pH electrode, or check the icon **PH** shows at LCD display.
2. Dip the electrode into the buffer solution pH 7. Stir gently and wait until the display stabilized.
Press and hold  button to enter calibration mode until the display appears icon **CAL**, and then flash 7.00. When the display stop flashing and indicates "SA", then "End" while calibration is ending, and return to measurement mode.